


TIP Sheet – How to Access Point of Use and View Implant History

Accessing Point of Use


1. Log into Powerchart




2. Select patient from search bar in Powerchart
3. Open Point of use from **Supply Point of Use** in Powerchart




4. POU opens to default performing location.

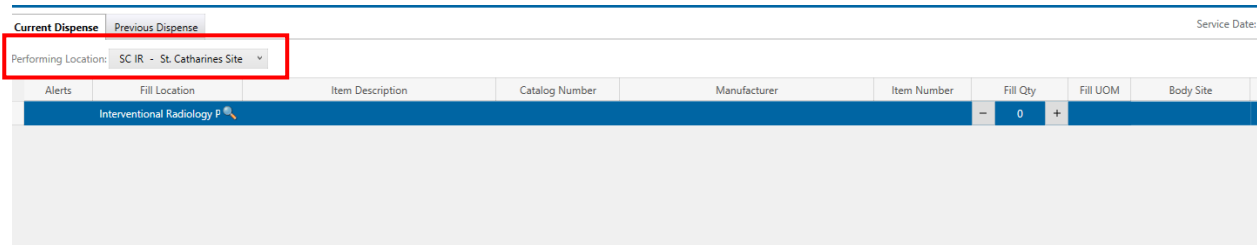

5. Scan barcode: Implant will come on the screen

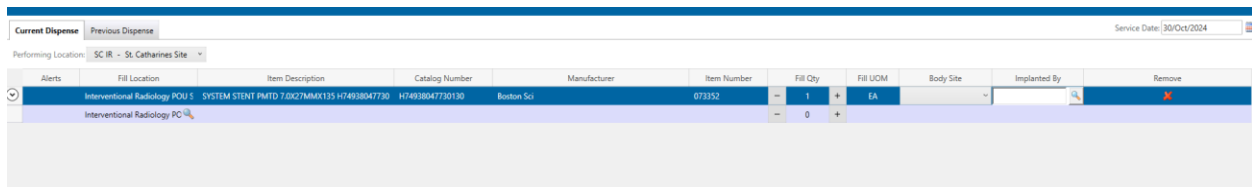


6. If unable to Scan click **Item search** on the bottom left side of the screen

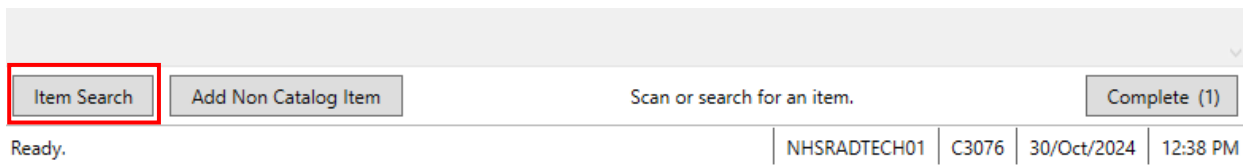


Ready. NHSRADTECH01 C3076 30/Oct/2024 12:38 PM

a. From **Item Search** a new window will open allowing you to search and Select your desired item(s). Press the **OK** button on the bottom right of the window to proceed.

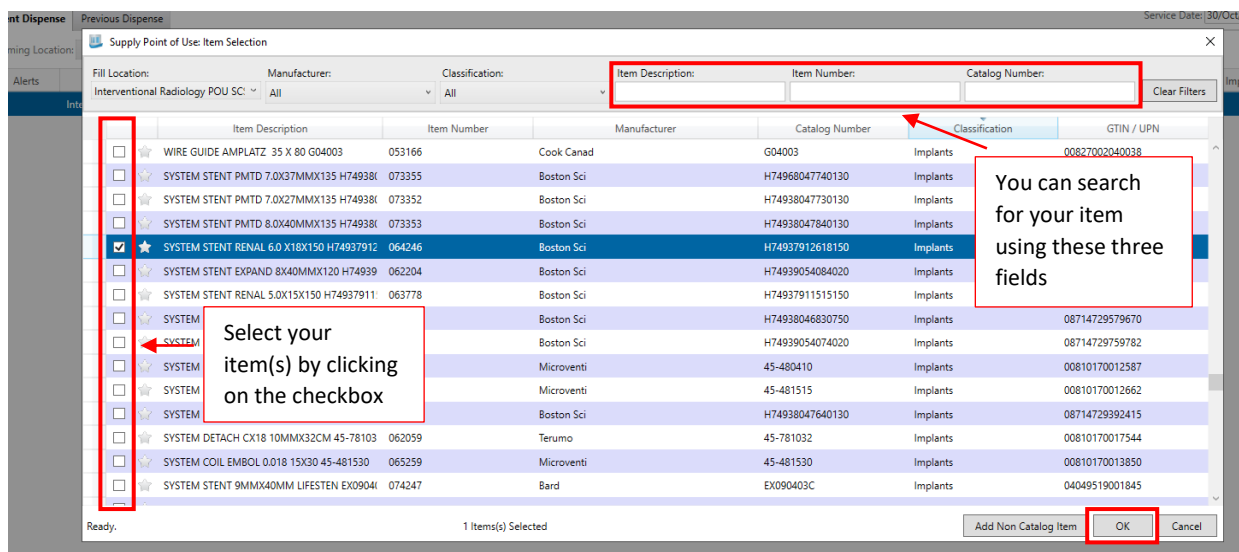

Item Description	Item Number	Manufacturer	Catalog Number	Classification	GTIN / UPN
WIRE GUIDE AMPLATZ 35 X 80 G04003	053166	Cook Canad	G04003	Implants	00827002040038
SYSTEM STENT PMTD 7.0X37MMX135 H74938C	073355	Boston Sci	H74968047740130	Implants	
SYSTEM STENT PMTD 7.0X27MMX135 H74938C	073352	Boston Sci	H74938047730130	Implants	
SYSTEM STENT PMTD 8.0X40MMX135 H74938C	073353	Boston Sci	H74938047840130	Implants	
SYSTEM STENT RENAL 6.0 X18X150 H74937912	064246	Boston Sci	H74937912618150	Implants	
SYSTEM STENT EXPAND 8X40MMX120 H74939	062204	Boston Sci	H74939054084020	Implants	
SYSTEM STENT RENAL 5.0X15X150 H74937911	063778	Boston Sci	H74937911515150	Implants	
SYSTEM		Boston Sci	H74938046830750	Implants	08714729579670
SYSTEM		Boston Sci	H74939054074020	Implants	08714729759782
SYSTEM		Microventi	45-480410	Implants	00810170012587
SYSTEM		Microventi	45-481515	Implants	00810170012662
SYSTEM		Boston Sci	H74938047640130	Implants	08714729392415
SYSTEM DETACH CX18 10MMX32CM 45-78103	062059	Terumo	45-781032	Implants	00810170017544
SYSTEM COIL EMBOL 0.018 15X30 45-481530	065259	Microventi	45-481530	Implants	00810170013850
SYSTEM STENT 9MMX40MM LIFESTEN EX0904C	074247	Bard	EX090403C	Implants	04049519001845

b. Some items will prompt you to fill out the **Lot Number** and **Expiration Date** of the item before proceeding. These can be scanned or manually entered into the highlighted fields. Press **OK** to proceed or **Cancel** if you need to go back and make any changes to your selection.

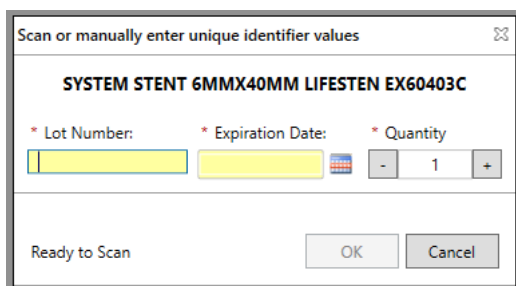


Scan or manually enter unique identifier values

SYSTEM STENT 6MMX40MM LIFESTEN EX60403C

* Lot Number: * Expiration Date: * Quantity

Ready to Scan OK Cancel

7. If unable to find items: click **Add Non Catalog Item** from the bottom left side of the screen to quickly add an item.

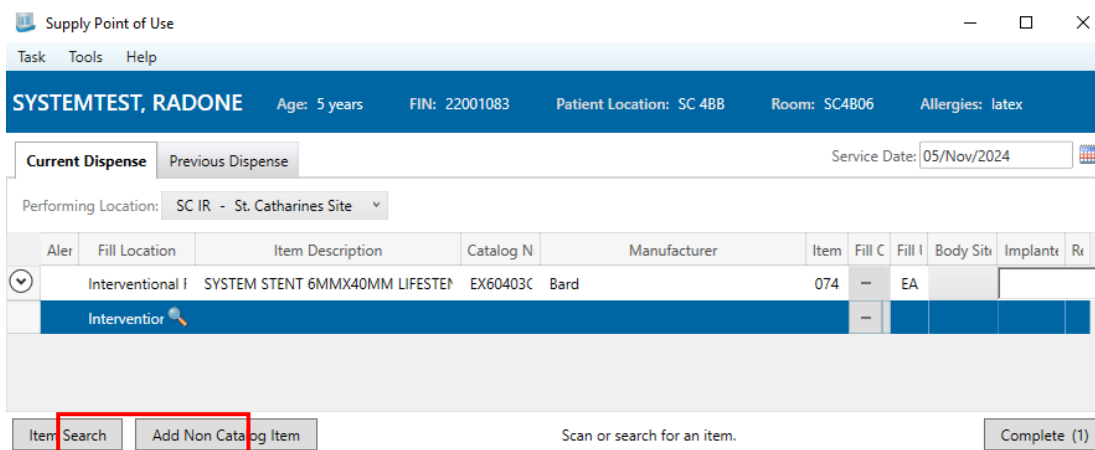

Supply Point of Use

Task Tools Help

SYSTEMTEST, RADONE Age: 5 years FIN: 22001083 Patient Location: SC 4BB Room: SC4B06 Allergies: latex

Current Dispense Previous Dispense Service Date: 05/Nov/2024


Performing Location: SC IR - St. Catharines Site

Aler	Fill Location	Item Description	Catalog N	Manufacturer	Item	Fill C	Fill I	Body Site	Implants	Re
Interventional I		SYSTEM STENT 6MMX40MM LIFESTEP	EX60403C	Bard	074	--	EA			

Interventional I

Item Search Add Non Catalog Item Scan or search for an item. Complete (1)

- a. Type or scan in details of implants. Click **OK** once complete, or **Cancel** to go back.

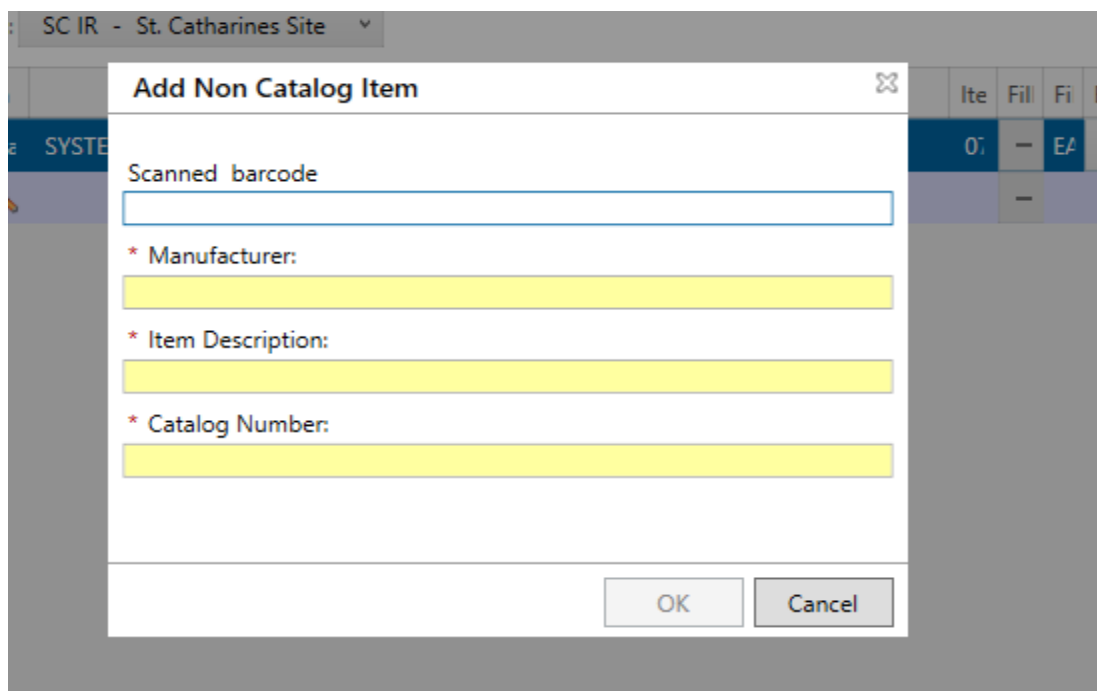

SC IR - St. Catharines Site

Add Non Catalog Item


Scanned barcode

* Manufacturer:

* Item Description:

* Catalog Number:


OK Cancel

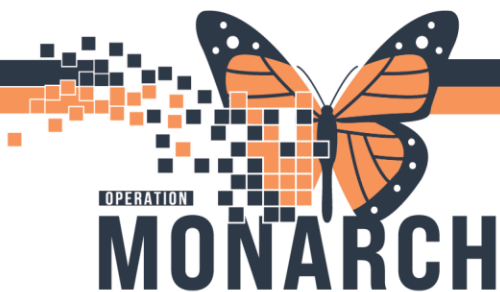


TIP SHEET

HOSPITAL INFORMATION SYSTEM (HIS)

- If an implant needs to be **removed**, click on the item to highlight it, then click the red cross to remove it.

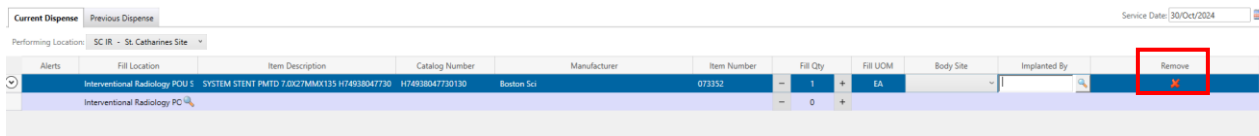

- Once you're finished making changes, click **Complete** on the bottom right corner. The Supply Point of Use window will then close.

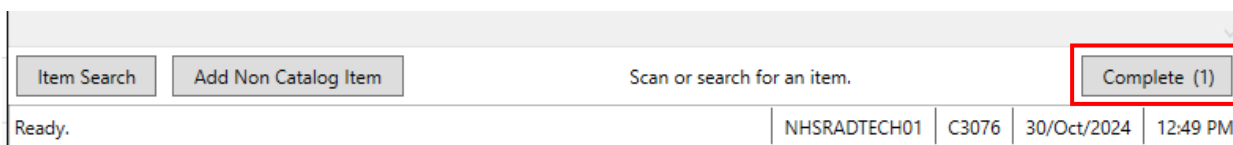


If an implant has to be returned or it has been wasted:


- Log into Powerchart




- Open Point of use from **Supply Point of Use** in Powerchart



- POU opens to default performing location.

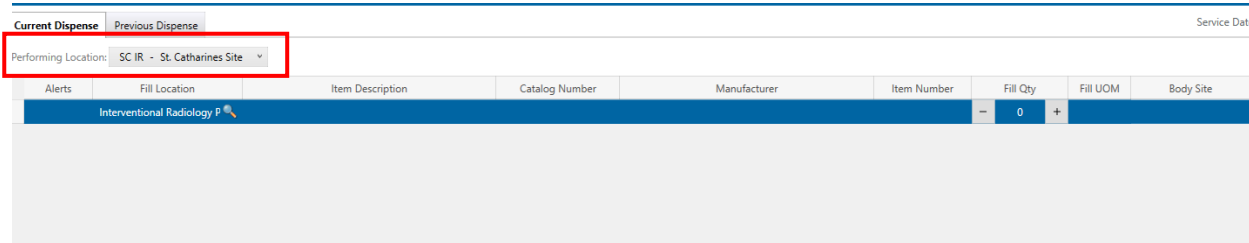

4. Select Previous Dispense tab to see your previous implants.

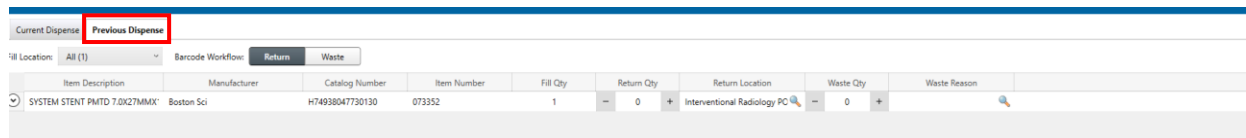


Current Dispense: **Previous Dispense**

Fill Location: All (1) Barcode Workflow: **Return** Waste


Item Description	Manufacturer	Catalog Number	Item Number	Fill Qty	Return Qty	Return Location	Waste Qty	Waste Reason
SYSTEM STENT PMTD 7.0K27MMX	Boston Sci	H74938047730130	073352	1	0	Interventional Radiology PC	0	

5. Select the drop-down arrow beside the item you would like to make updates to.



Item Description	Manufacturer	Catalog Number	Item Number	Fill Qty	Return Qty	Return Location	Waste Qty	Waste Reason
SYSTEM STENT PMTD 7.0K27MMX	Boston Sci	H74938047730130	073352	1	0	Interventional Radiology PC	0	Wasted

6. Manually return/waste item by selecting plus icon on either the Return Qty or Waste Qty. To make changes, just press the minus icon on either option to remove that selection.

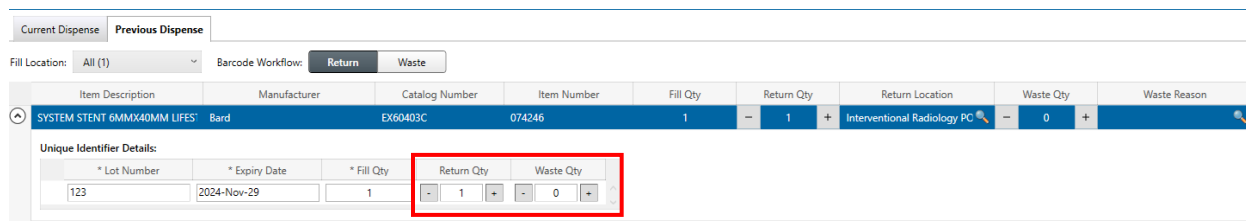

Current Dispense: **Previous Dispense**


Fill Location: All (1) Barcode Workflow: **Return** Waste

Item Description	Manufacturer	Catalog Number	Item Number	Fill Qty	Return Qty	Return Location	Waste Qty	Waste Reason
SYSTEM STENT 6MMX40MM LIFES	Bard	EX60403C	074246	1	1	Interventional Radiology PC	0	

Unique Identifier Details:

* Lot Number	* Expiry Date	* Fill Qty	Return Qty	Waste Qty
123	2024-Nov-29	1	1	0

a. If using a scanner: select the Return/Waste buttons at the top of the screen to configure your scanner to either automatically log the item as returned or wasted.

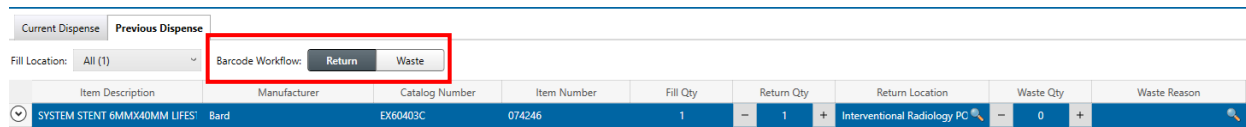

Current Dispense: **Previous Dispense**

Fill Location: All (1) Barcode Workflow: **Return** Waste

Item Description	Manufacturer	Catalog Number	Item Number	Fill Qty	Return Qty	Return Location	Waste Qty	Waste Reason
SYSTEM STENT 6MMX40MM LIFES	Bard	EX60403C	074246	1	1	Interventional Radiology PC	0	


7. Click Complete on the bottom right corner of the window to log in your changes and close out of Supply Point of Use.

Viewing the Implant History in Powerchart


1. Log into Powerchart



2. Select patient from search bar in Powerchart
3. Select the **Imaging Synopsis** M-Page from the left hand side of your screen

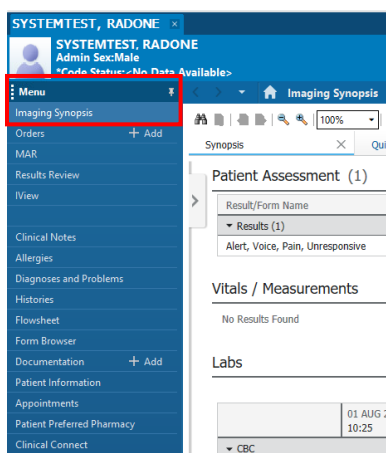

4. Hover over the > arrow on the left side to slide out the subsection headers of the **Imaging Synopsis** page to quickly go to **Implant History**. You can also simply scroll down until you reach that section of the **Imaging Synopsis**.

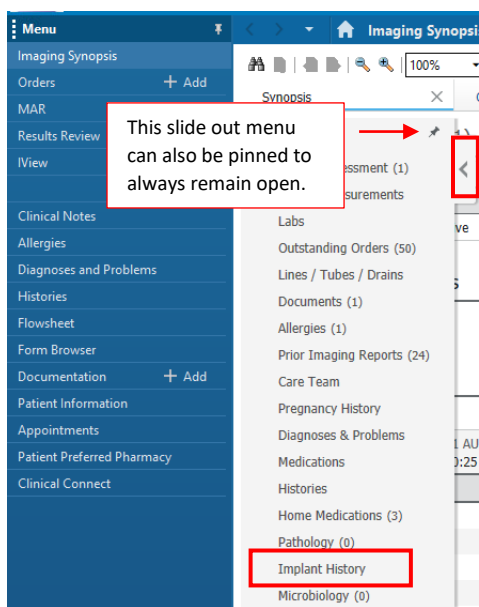



TIP SHEET

HOSPITAL INFORMATION SYSTEM (HIS)

5. From the **Implant History** you can view all of the previous implants on this patient.
6. You can filter your view to see only Active, Active + Explanted, or Inactive Implants on this patient

Implant History

Implant Date	Description	Explant Date	Type	Materials	Site	HR Classification	Source
▼ Active							

Implant History

Implant Date	Description	Explant Date	Type	Materials	Site	HR Classification	Source
▼ Inactive							
05 NOV 2024	SYSTEM STENT GOREKAORHM LIFESTEN EXBO...	--	Non Biological	--	--	--	Departmental Scan